



System 1

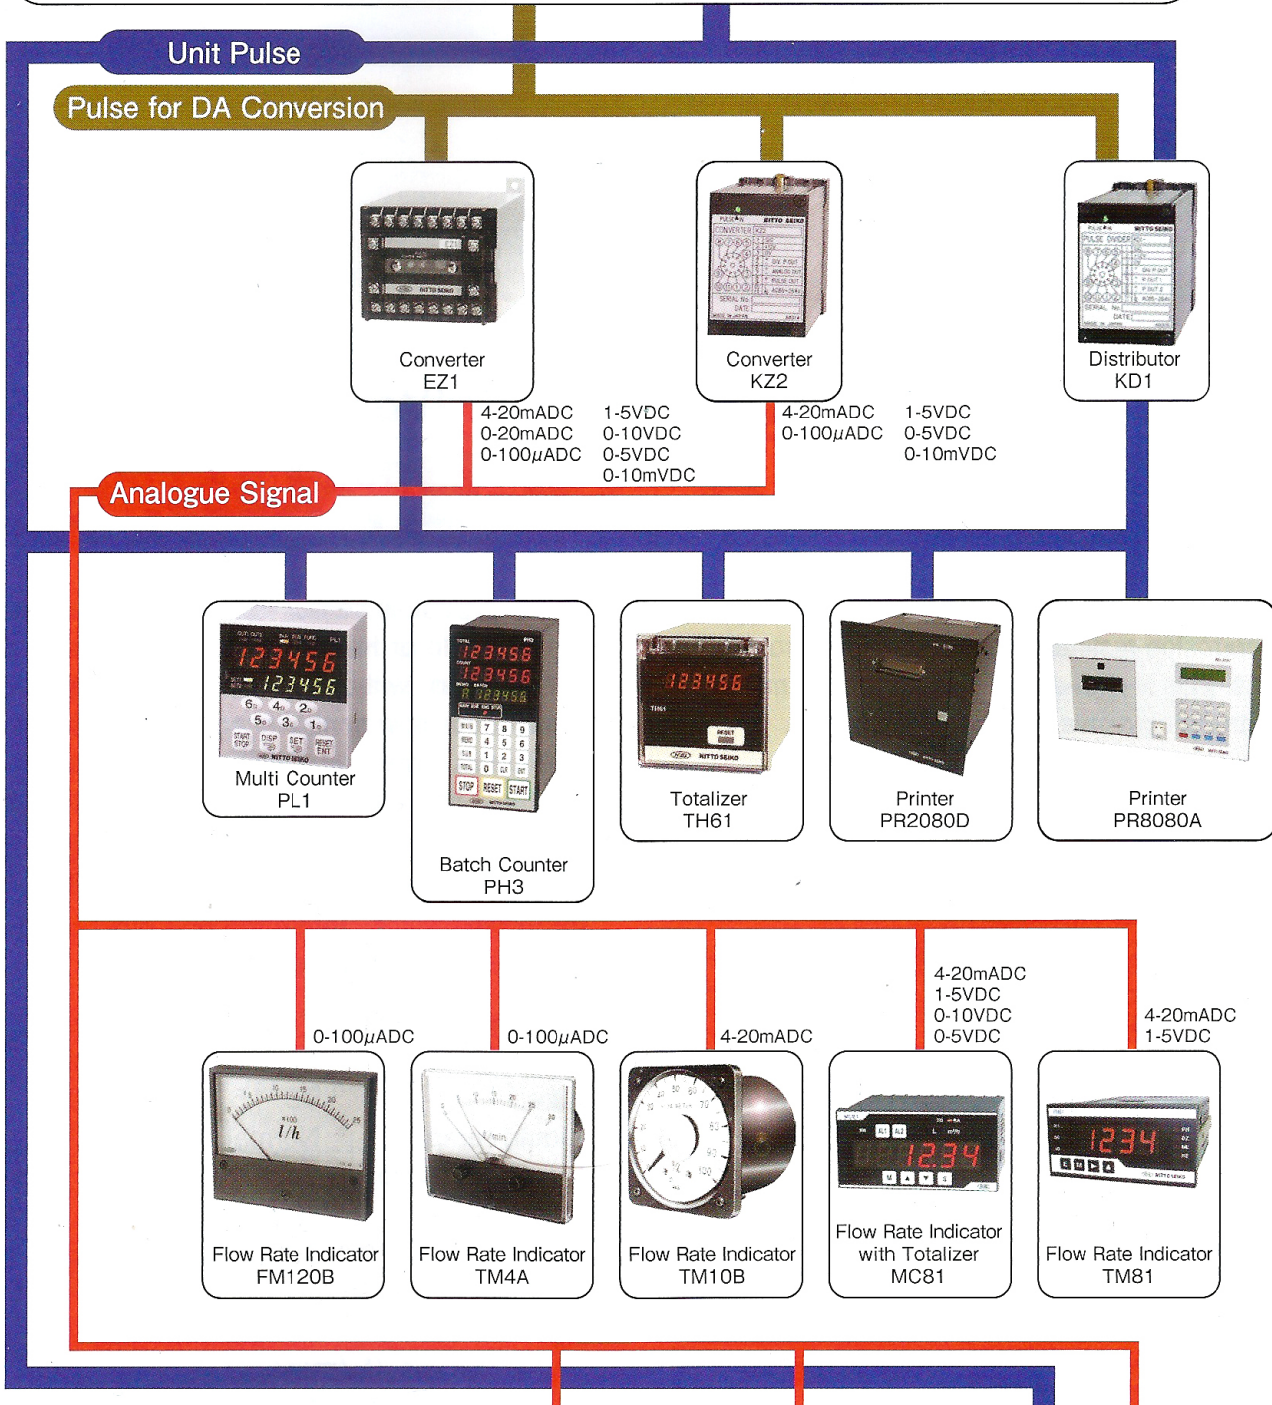

for DA conversion is output by high frequency generator.
 pulse is output by reed switch, high frequency generator, or photoelectric pulse generator.

1. Converter and instruments need power supply of 100V or 200V AC
2. As for the details of converter and instruments, please refer to the special catalog or specification sheet.

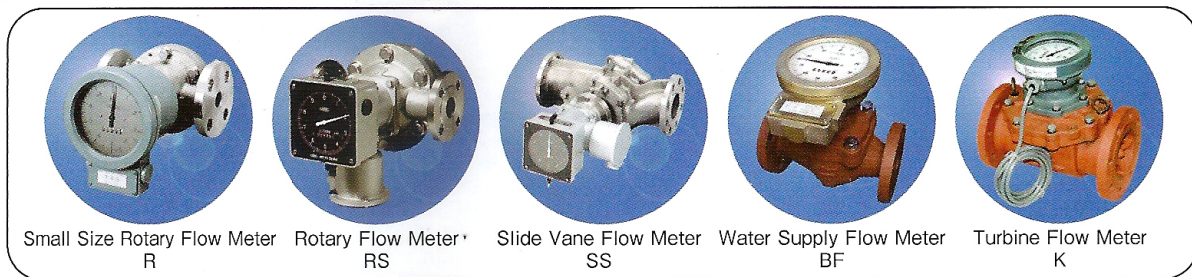